



INTERNATIONAL ATOMIC ENERGY AGENCY
UNITED NATIONS EDUCATIONAL, SCIENTIFIC AND CULTURAL ORGANIZATION
INTERNATIONAL CENTRE FOR THEORETICAL PHYSICS
I.C.T.P., P.O. BOX 586, 34100 TRIESTE, ITALY, CABLE: CENTRATOM TRIESTE



H4-SMR 471/09

COLLEGE ON MEDICAL PHYSICS

10 - 28 SEPTEMBER 1990

METHODS FOR PRODUCING BIOMEDICAL IMAGES
THROUGH RECONSTRUCTION FROM PROJECTIONS

Dr. Enrico M. Staderini

METHODS FOR PRODUCING BIOMEDICAL IMAGES
THROUGH RECONSTRUCTION FROM PROJECTIONS

Enrico M. Staderini

Universita degli Studi "La Sapienza"
Roma
Italy

TABLE I: PHYSICS AND TECHNOLOGY OF CT APPLICATION

The physics and technology of computed tomography (CT) applications is summarized in Table I (modified from [1]). In that table the emanations (i.e. the sources of energy) used to test the object are listed along with the measured physical quantities and the transducers most usefully employed.

This is to remember the large number of today offered technological possibilities to perform a computed tomography, as well as the vast application field for the various methods of image reconstruction from projections.

Most used emanations are X-rays, acoustic waves, magnetic and radio-frequency electro-magnetic fields which have permitted the realization of practical systems for CT, echography and NMR (nuclear magnetic resonance) tomography.

<u>Emanations used</u>	<u>Densities measured</u>	<u>Transducers employed</u>	<u>Applications</u>
X-rays	attenuation coefficients	X-ray sources; scintillation detectors	Diagnostic Radiology (DR); Nondestructive Testing (NDT)
Gamma-rays	concentration of radio-labeled substance	scintillation counters	DR; Nuclear Medicine
Compton scattered X-rays, Gamma-rays	electron density or distribution of atomic number	X-ray sources; scintillation counters	DR; NDT; X-ray crystallography
Heavy particles	scattering/absorption cross section	linear accelerators; stacked detectors	DR; NDT
Electron beams	Schrodinger potential distribution	electron guns; film; photomultiplier / TV	Microscopy
Acoustic waves	attenuation; refractive index; acoustic impedance	electro-mechanical devices	DR; NDT; Geological Prospecting (GP)
Low-frequency electric currents	electr. conductivity distribution	electrodes	Imaging of blood vessels; GP; NDT
Magnetic fields	distribution of nuclear spins; blood flow	magnets; RF coils; magnetometers	Nuclear Magnetic Resonance (NMR); Magneto-Hydro-Dynamic (MHD)
Radio-frequency fields	electron spins; permittivity and conductivity distribution	capacitors; coils; antennas; horns	NMR; Mapping
Spatially incoherent electromagnetic radiations	volume temperature distributions; celestial brightness distributions	horns; antennas; telescopes	Mapping temperature distrib.; Astronomical imaging

TECHNIQUES APPLIED FOR REMOTE-SENSING CT

Regarding the degree of control we have on the sources employed, three main tomography techniques can be defined.

When the sources are emitting from inside the body, nothing the experimenter can do over them but remote sense their emanations coming from the body. This operation is called remote sensing computed tomography (Table II).

Another aspect of computed tomography concerns the use of sources applied externally of the body and measuring the emanations passed through the object. This is the remote probing computed tomography (Table III).

In combined probing-sensing computed tomography we deal with emanations generated from sources internally placed in the body after a sort of stimulation or excitation from externally applied emanations (Table IV).

Single Photon Emission Computed Tomography (SPECT)

Positron Emission Tomography (PET)

Super Synthesis
(e.g. Earth rotation synthesis telescope)

TABLE II

TECHNIQUES APPLIED FOR REMOTE-PROBING CT

Transmitted X-rays (Computed Tomography CT)
Transmitted Heavy Particles
Reflected Ultrasound Transmitted Ultrasound
Reflected Radiowaves (RADAR)
Electrical Impedance
Electron Microscopy

TABLE III

TECHNIQUES APPLIED FOR PROBING-SENSING CT

Nuclear Magnetic Resonance (NMR)
Corrected Emission
Uncorrected Compton Scatter
Corrected Compton Scatter
Magneto-Hydro-Dynamic

TABLE IV

where $T(s) = (1 - s^2)^{1/2}$ $|s| < 1$ [7]

and $p(s, \theta) = 0$ $|s| > 1$ [8]

Please note that we are not in presence of a polar coordinate system as:

$$p(0, \theta_1) = p(0, \theta_2) \quad [9]$$


Note also the periodism:

$$p(s, \theta) = p(-s, \theta + \pi) \quad [10]$$

INTERACTION WITH MATTER


Figure 2 shows the effect of linear attenuation of a beam of intensity I_0 when passing through an absorbing medium. The linear attenuation coefficient μ is a function of the energy of the photons and of the atomic number and density of the matter. If the specimen is not homogeneous, then μ is also a function of the spatial coordinates. Moreover, if the beam is polychromatic, only a mean of μ over present energies can be measured.

At the bottom of fig. 2 the experimental projection function is determined as a function of the measured quantities.

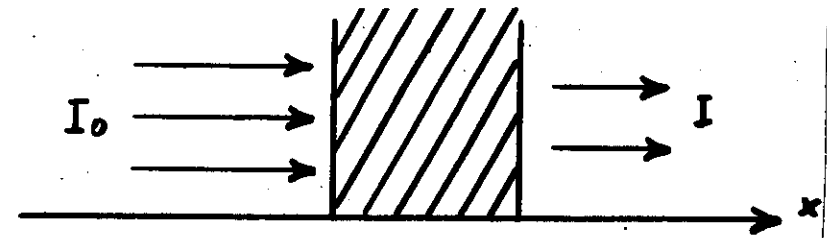

$$\frac{dI}{dx} = -\mu I \quad I = I_0 e^{-\mu x}$$

$$\mu = f(E, Z, \rho, \text{polariz.}, x, y)$$

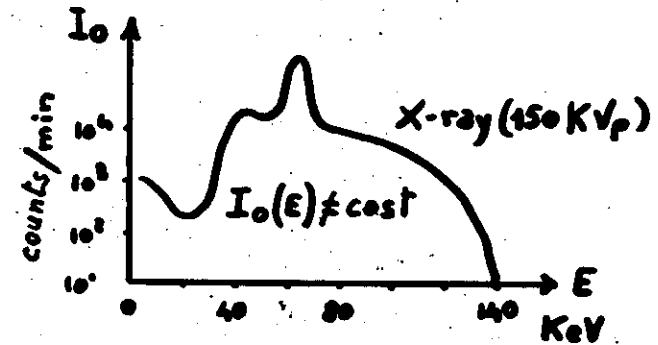

$$I(s, \theta) = I_0 e^{-\int_{s, \theta} \mu(x, y) dt}$$

$$p(s, \theta) = \ln\left(\frac{I_0}{I(s, \theta)}\right)$$

fig. 2

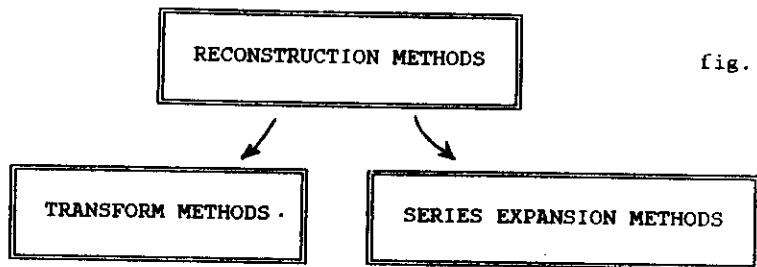


fig. 3

TRANSFORM METHODS

In the transform methods the problem of reconstruction from projections is faced by formulating a mathematical model in which known and unknown quantities are functions whose arguments come from a continuum of real numbers. Then solving for the unknown function with an inversion formula and adapting this formula for discrete or noisy data [2].

The generalized projection theorem is the basis for understanding the two most important transform methods of reconstruction. For any given angle θ the following relation holds:

$$\int_{-1}^1 p(s, \theta) w(s) ds = \iint_{\mathcal{R}} f(x, y) w(x \cos \theta + y \sin \theta) dx dy \quad [11]$$

The proof is simply obtained by substituting the left side using [6] and then converting from rotated coordinates using [3] and [4].

An obvious application of this theorem is obtained by using $\exp(-i2\pi Rs)$ as $w(s)$. In this case it will follow that the 1-D Fourier transform of the projection at angle θ is equal to the central slice, at the same angle, of the 2-D Fourier transform of

the resulting image. This theorem is often called as the projection-slice theorem or the central-section theorem and it allows for practical reconstruction algorithm using Fourier transform.

Now let us consider the last theorem which can be stated in the following way:

$$\hat{p}(R, \theta) = \hat{f}(R \cos \theta, R \sin \theta) \quad [12]$$

It is the central-section theorem where $\hat{p}(R, \theta)$ is the 1-D Fourier transform of the projection $p(s, \theta)$ with respect to the first variable.

Taking the inverse Fourier transform of [12] we obtain:

$$f(x, y) = \int \int_{-\infty}^{\infty} \hat{p}(R, \theta) e^{i2\pi R(x \cos \theta + y \sin \theta)} |R| dR d\theta \quad [13]$$

As the following identity holds:

$$\hat{p}(R, \theta_m) = \int_{-1}^1 p(s, \theta_m) e^{-i2\pi R s} ds \quad [14]$$

for the projection angle θ_m , and considering that we have to deal with sampled data (i.e. we have to use a window function $W(R)$)

to obtain a band limited reconstructed image $f_B(x, y)$ we have:

$$f_B(x, y) = \int \int_{-\frac{1}{2}AS}^{\frac{1}{2}AS} \hat{p}(R, \theta) w(R) e^{i2\pi R(x \cos \theta + y \sin \theta)} |R| dR d\theta \quad [15]$$

Using [14] we obtain:

$$f_B(x, y) = \int \int_{-\frac{1}{2}AS}^{\frac{1}{2}AS} \int_{-1}^1 p(s, \theta) e^{-i2\pi R s} w(R) e^{i2\pi R(x \cos \theta + y \sin \theta)} |R| ds dR d\theta \quad [16]$$

now considering the following functions:

$$q(s) = \int_{-\frac{1}{2}AS}^{\frac{1}{2}AS} |R| w(R) e^{i2\pi R s} dR \quad [17]$$

$$\hat{q}(R) = |R| w(R) \quad [18]$$

we have:

$$f_B(x, y) = \int \int_{-1}^1 p(s, \theta) q(x \cos \theta + y \sin \theta - s) ds d\theta \quad [19]$$

after having interchanged the order of integration over s and R .

Note now that the problem of reconstructing the function $f_B(x,y)$ may be split into two parts.

At first we can integrate over s and then integrate over θ .

We obtain:

$$\tilde{p}(s',\theta) = \int_{-1}^1 p(s,\theta) q(s'-s) ds \quad [20]$$

which is mathematically a convolution of $p(s,\theta)$ using the function q as a convolution kernel.

Then we have:

$$f_B(x,y) = \int_0^\pi \tilde{p}(x \cos \theta + y \sin \theta, \theta) d\theta \quad [21]$$

in which the parameters of the function p are nothing but the parameters of a ray passing through the point (x,y) at angle θ . The [21] is simply the backprojection of all convolved projections.

The method so described is the well-known filtered back-projection (as the convolution is nothing but a filter) or convolution back-projection method.

The errors arising from the reconstruction methods are mainly due to technological limitations. These come from:

- a) insufficient sampling of the projection
- b) errors in estimation of \hat{p}
- c) errors in the Fourier domain (interpolation, sampling).


As regards the comparison between the Fourier reconstruction and the convolution back-projection one it is to be said that the latter has a far better performance. The Fourier

reconstruction algorithm has its weakness in the inelegant 2-D interpolation required, producing images of bad quality. The Fourier algorithm, on the other hand, has the potentiality to be performed with less computational effort respect to the convolution back-projection and this makes the Fourier algorithm worth of even more investigation effort.

FINITE SERIES-EXPANSION METHODS

In this family of reconstruction methods we are formulating a model which relates a finite set of known numbers with a finite set of unknown numbers. The resulting system of equations is then solved in a numeric way.

The line integral of the unknown attenuation function along the path of the ray can be expressed as in fig. 4, where it is the sum of the products of the attenuation coefficient of each pixel multiplied by the length of the intersection of the ray i with the squared pixel j .

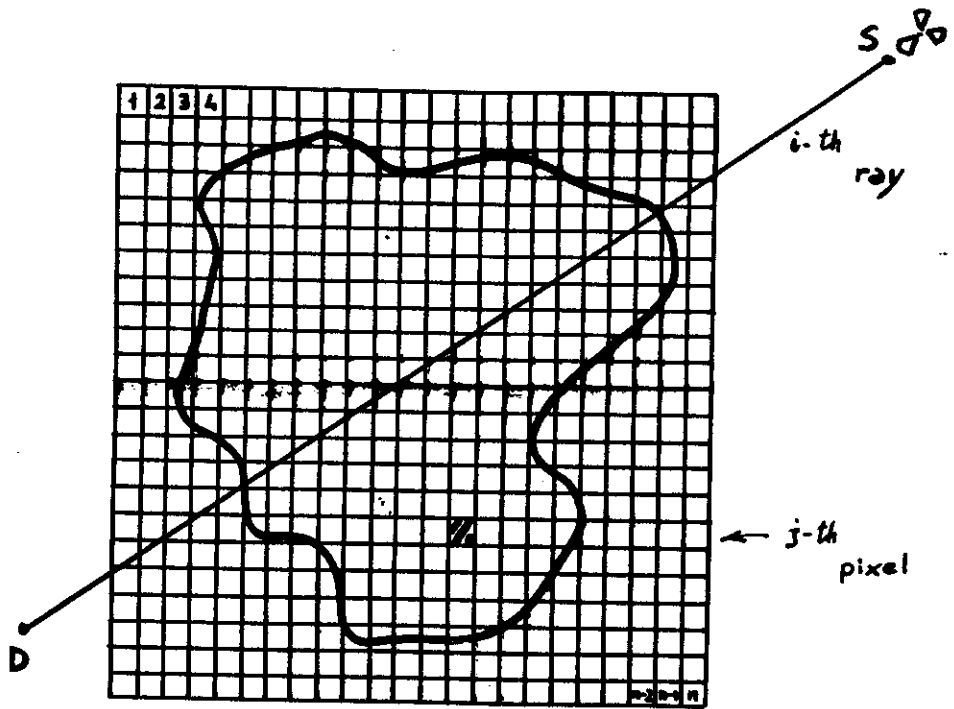

$$\sum_{j=1}^m x_j a_{ij} \approx y_i \quad i=1 \dots m$$

fig. 4

In different words let us consider a set of basis functions in polar coordinates in plane:

$$\{b_j(r, \phi)\}_{j=1}^m \quad [22]$$

where

$$b_j(r, \phi) = \begin{cases} 1 & (r, \phi) \in \text{pixel } j \\ 0 & \text{otherwise} \end{cases} \quad [23]$$

The digitalized image is then represented as:

$$\hat{f}(r, \phi) = \sum_{j=1}^m \kappa_j b_j(r, \phi) \quad [24]$$

Using a set of continuous functionals which assign to any picture $f(r, \phi)$ a real number $R_i f$, we can say that $R_i f$ is the line integral of $f(r, \phi)$ along the i -th ray.

Then:

$$y_i \approx R_i f \approx R_i \hat{f} = \sum_{j=1}^m \kappa_j R_i b_j(r, \phi) = \sum_{j=1}^m \kappa_j a_{ij} \quad [25]$$

so we obtain a set of equations:

$$y = A x \quad [26]$$

Unfortunately the number of pixel n and the number of rays m are in the order of 10^5 and the direct matrix inversion is not generally feasible.

One of the best known reconstruction technique is the Algebraic Reconstruction Technique (ART).

This is an iterative method where the image matrix x is initially assigned an arbitrary number. For each iteration the matrix x is corrected (updated) by taking into account only a single ray and only the pixels intercepted by that ray. The discrepancy is redistributed along the pixels intercepted.

In formulas:

$$x^0 \in \mathbb{R}^m \quad [27]$$

$$x^{k+1} = x^k + \frac{y_i - \langle a^i, x^k \rangle}{\|a^i\|^2} a^i \quad [28]$$

where

$$\langle a^i, x^k \rangle = \sum_{j=1}^m a_j^i x_j^k \quad ; \quad \|a^i\|^2 = \langle a^i, a^i \rangle \quad ; \quad a^i = (a_{ij})_{j=1}^m$$

The ART method, and those derived from that, are very useful in image reconstruction as they are feasible for various projective geometries.

They can also be used in high contrast images, when the reconstruction can use only a few directions of view, or when execution time is crucial.

REFERENCES

The following references are quite complete reviews giving a good perspective of reconstruction techniques and relative performances. The papers may be highly useful for better comprehension of methods here presented in general terms.

- [1] Bates R.H.T., Garden K.L., Peters T.M., "Overview of computerized tomography with emphasis on future developments", Proc. IEEE, vol. 71, pp. 356-372, March 1983.
- [2] Lewitt R.M., "Reconstruction algorithms: Transform methods", Proc. IEEE, vol. 71, pp. 390-408, March 1983.
- [3] Censor Y., "Finite series-expansion reconstruction methods", Proc. IEEE, vol. 71, pp. 409-419, March 1983.